


Endoscopic Brow and Temporal Midface Lifting

Instruments recommended by Thomas ROMO III, MD, FACS

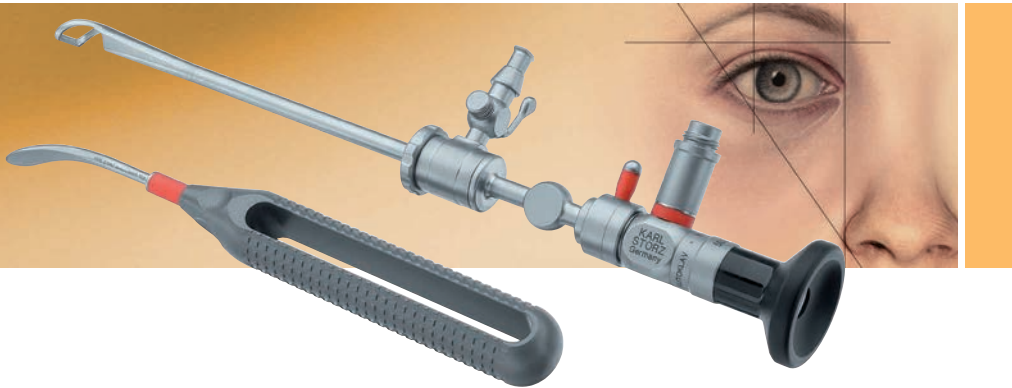

Endoscopic Brow and Temporal Midface Lift

Instruments recommended by Thomas ROMO III, MD, FACS

Rejuvenation of the midface and the forehead has become part of the standard treatment of the aging face. Surgical techniques for this area of the face have continually evolved with the emphasis on minimally invasive procedures. Endoscopic midface lift and forehead lift surgery is consistent with the minimally invasive approach.

The success of these procedures is based on the exact release of midface and periosteal attachments and the preservation of neurovascular structures. Reliable fixation devices ensure long-term tissue elevation and the proper position of healed facial structures.


Innovative instrumentation is required to meet the technical requirements for gentle yet reliable endoscopic treatment of midface and forehead soft tissue.

The new elevators and dissectors for the midface and forehead from KARL STORZ meet these requirements.


Continued innovation in this field will lead to new techniques as well as new surgical approaches and instruments.

I appreciate the support from this outstanding company.

Thomas ROMO III, M.D.

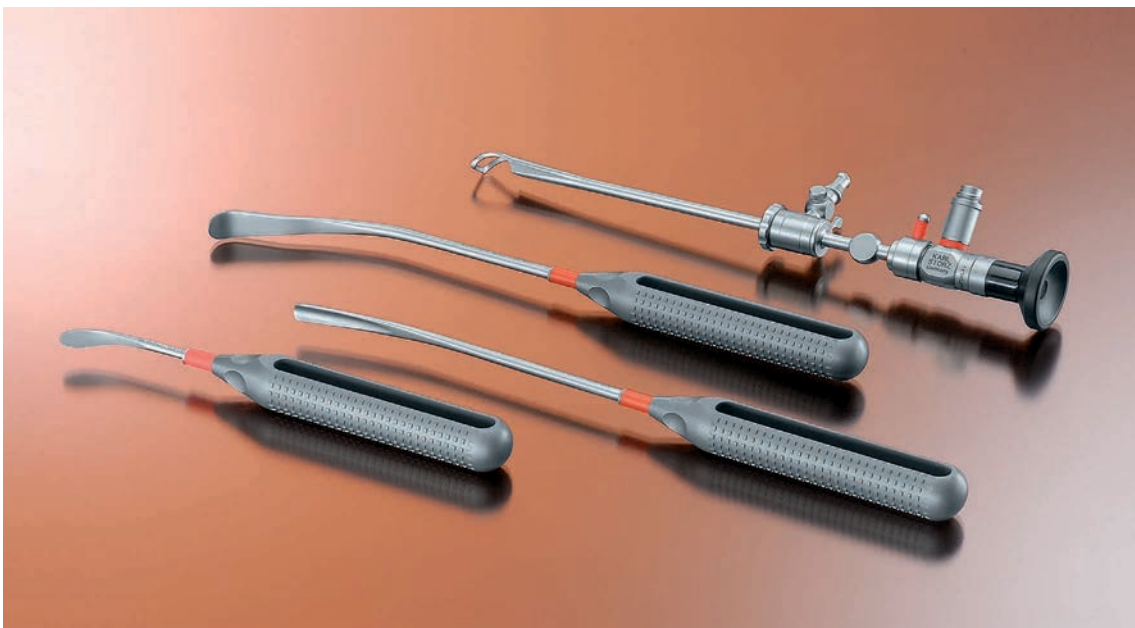

Instrumentation

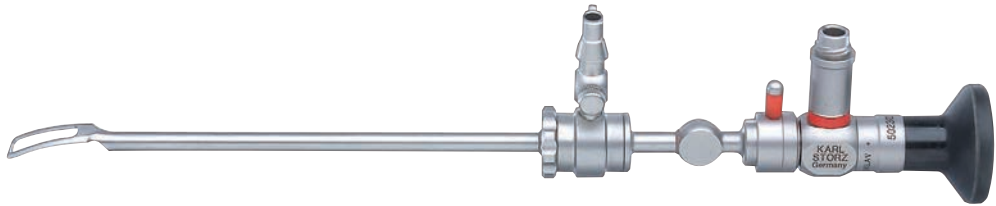

50230 BA **HOPKINS® Forward-Oblique Telescope 30°**, enlarged view, diameter 4 mm, length 18 cm, **autoclavable**, fiber optic light transmission incorporated, color code: red

50200 ES **Optical Dissector**, with distal spatula, fenestrated, large, sharp, for use with HOPKINS® telescopes 30°

Instruments for Brow and Temporal Midface Lift



58210 CA **Raspatory**, straight, spatula 12 x 12 mm, working length 15 cm



58210 MGA **Raspatory**, curved, curved upwards, upper part sharp, width 9 mm, working length 15 cm



58210 TKA **Raspatory**, curved, width 8 mm, working length 6 cm



58210 UKA **Raspatory**, slightly curved, hollow grinding, width 8 mm, working length 15 cm

Instrumentation



58210 CGA **Raspatory**, curved, spatula 12 x 12 mm, working length 15 cm

Further Instruments



58210 AGA **Raspatory**, curved, width 9 mm, working length 15 cm



58210 FGA **Raspatory**, curved, spatula curved, width 12 mm, working length 15 cm



58210 GGA **Raspatory**, curved, arc-shaped spatula, width 9 mm, working length 15 cm




58210 LGA **Raspatory**, curved, for lifting and dissecting the orbital rim periosteum, distal end of spatula 90° curved upwards, upper part sharp, width 9 mm, working length 15 cm




58210 WGA **Raspatory**, curved, triangular-shaped spatula, width 4 mm, working length 15 cm


Notes

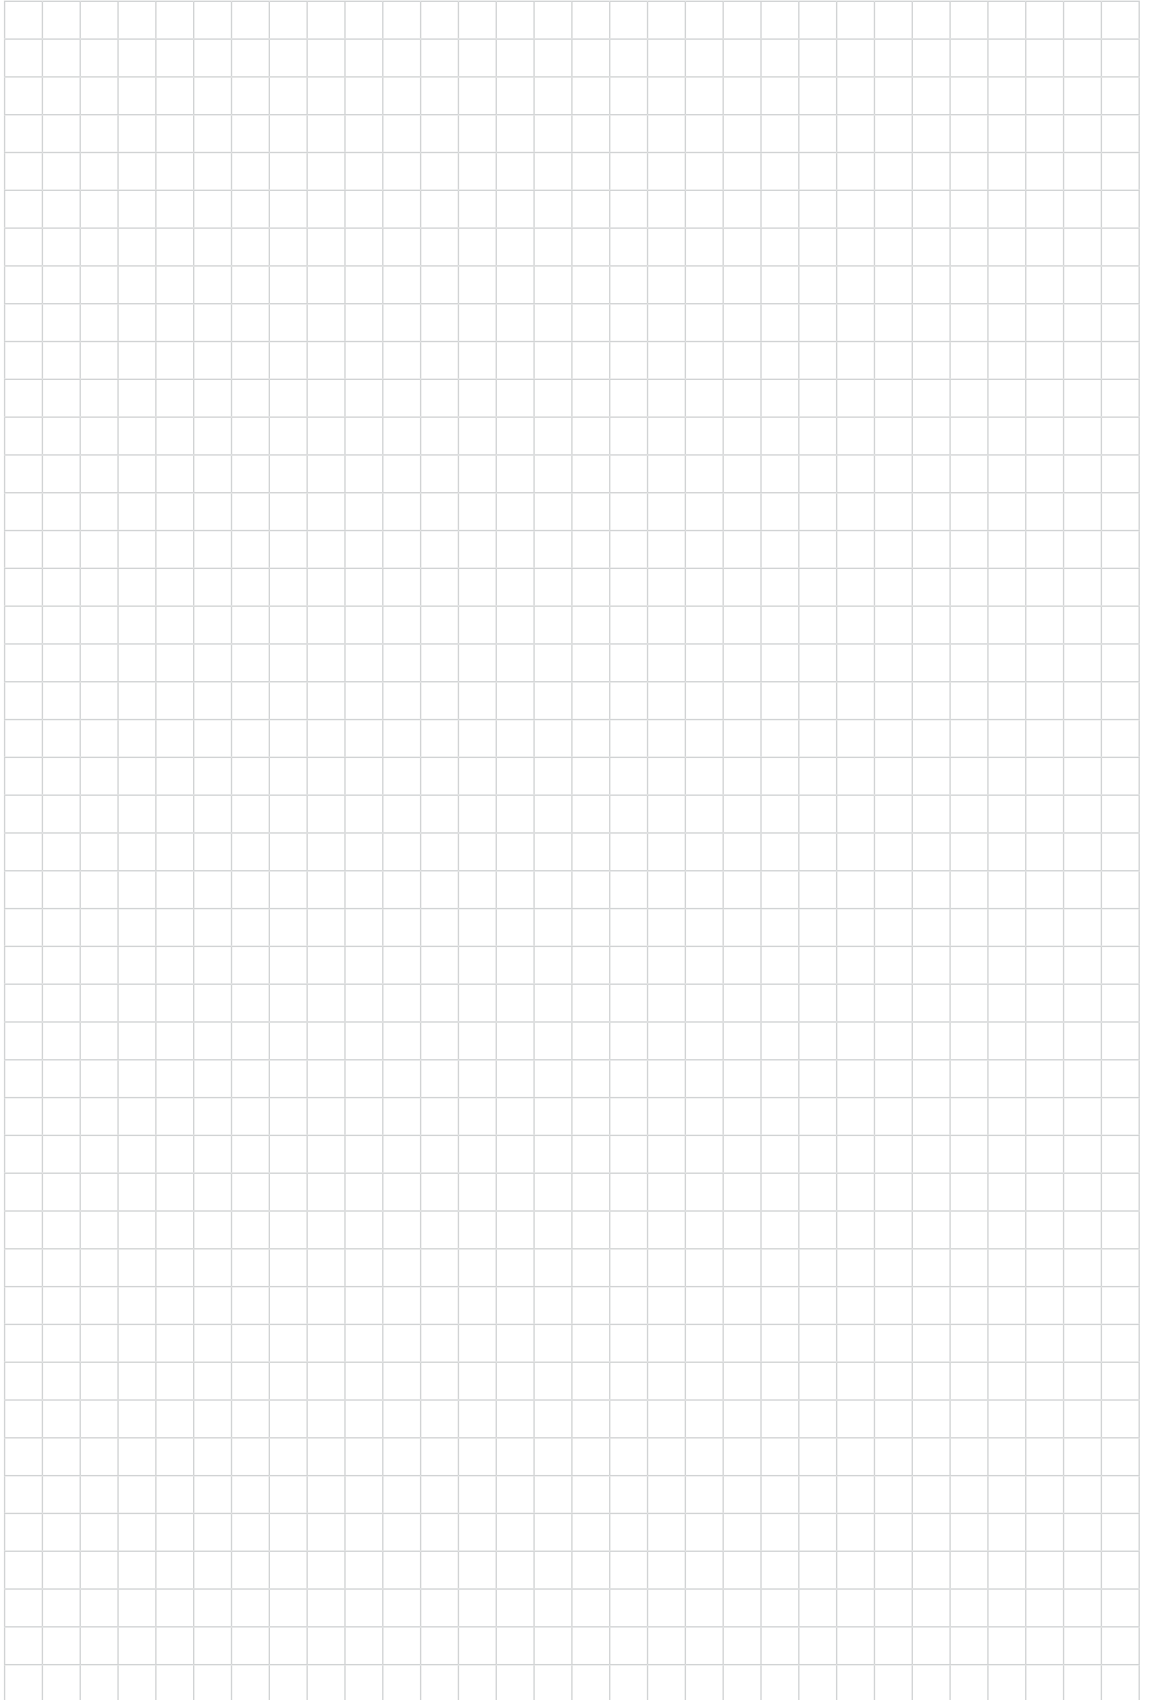

Notes

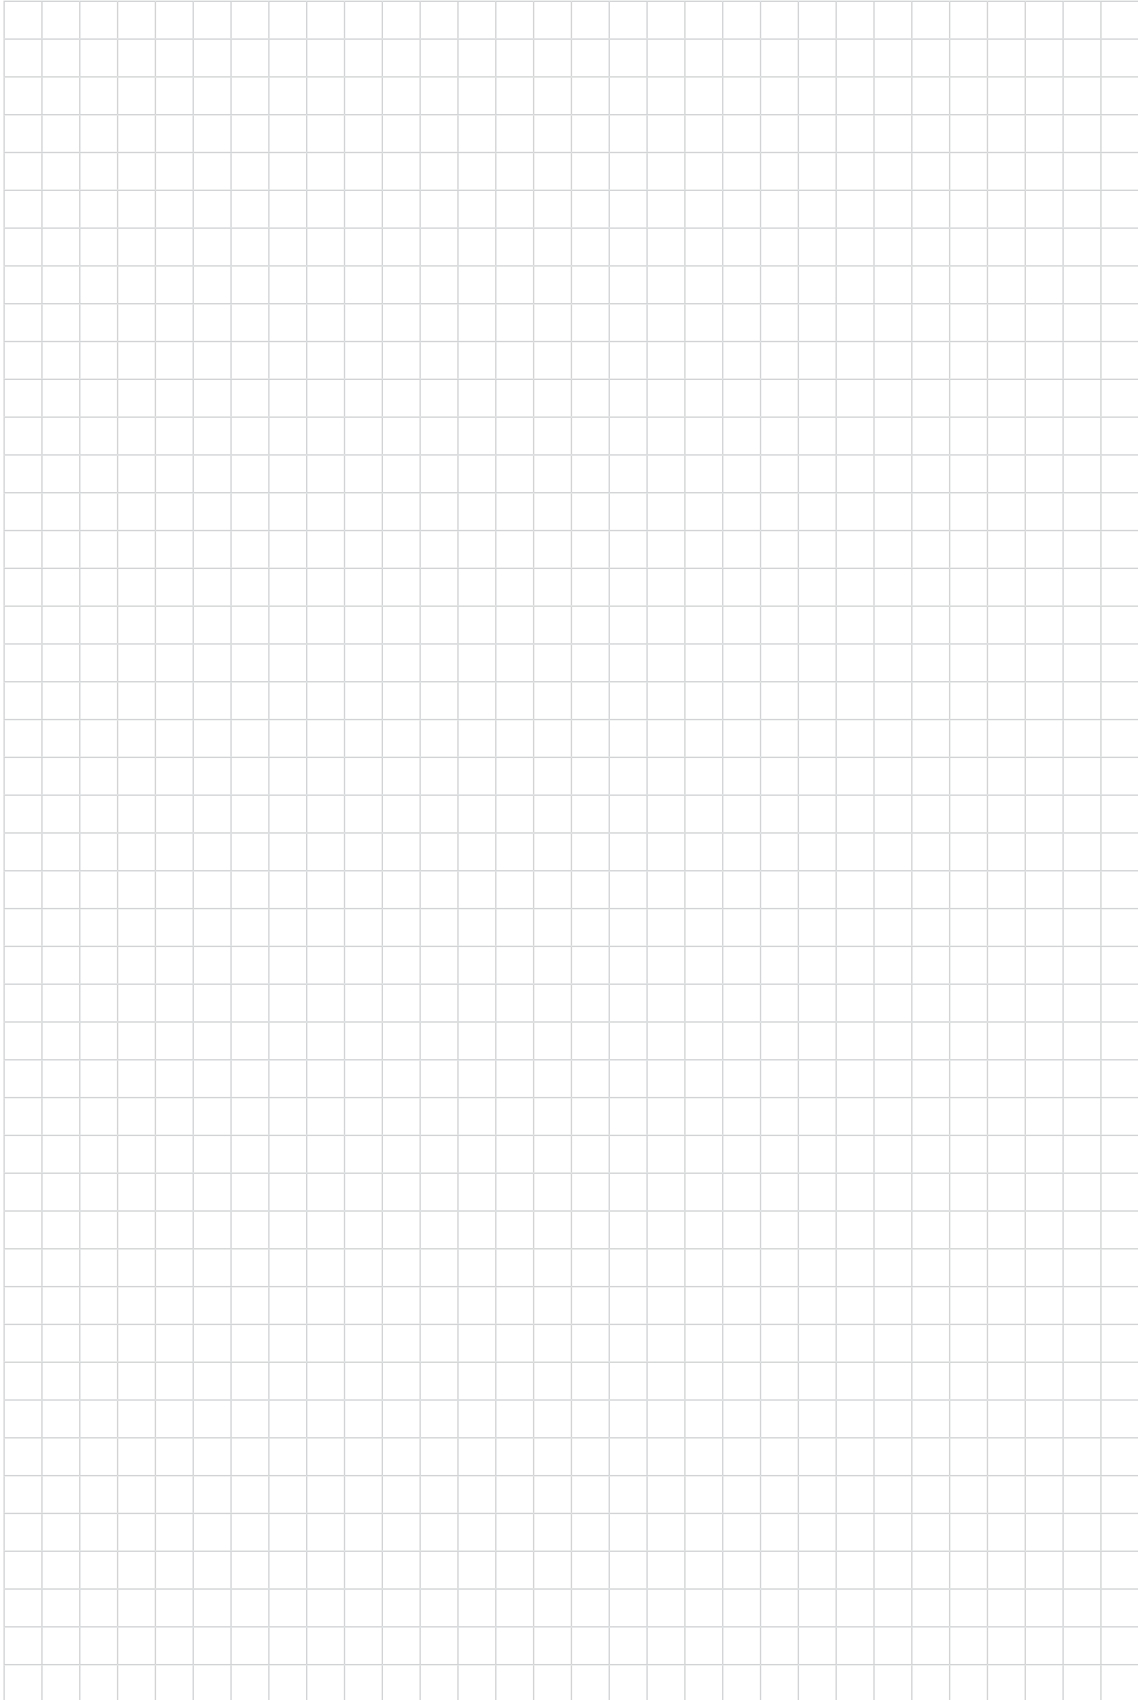

Notes

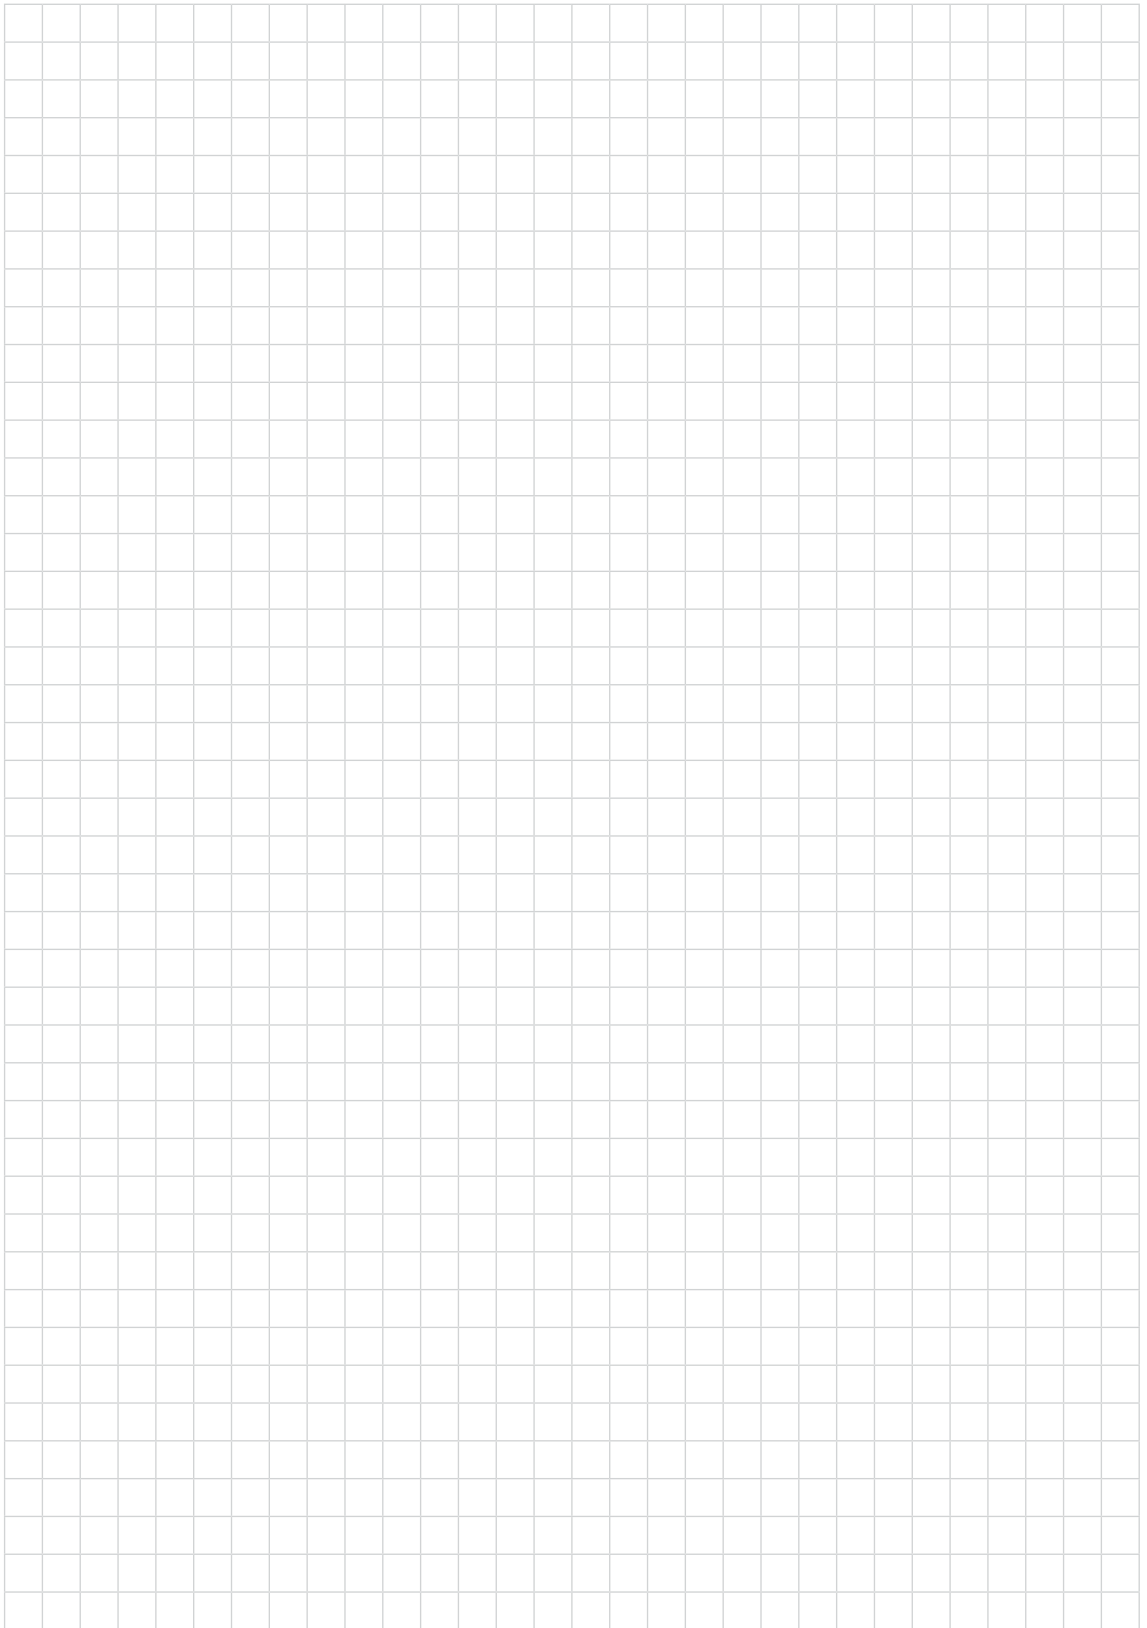

It is recommended to check the suitability of the product for the intended procedure prior to use.

STORZ
KARL STORZ—ENDOSKOPE
THE DIAMOND STANDARD

KARL STORZ SE & Co. KG
Dr.-Karl-Storz-Straße 34, 78532 Tuttlingen/Germany
Postfach 230, 78503 Tuttlingen/Germany
Phone: +49 (0)7461 708-0
Fax: +49 (0)7461 708-105
E-Mail: info@karlstorz.com
www.karlstorz.com

 Health
made in Germany
www.health-made-in-germany.com